


RLWS *Mass Value* CERTIFICATE

Contractor: G T Michelli
 130 Brookhollow Esplanade
 Harahan, LA 70123 5102

Purchase Order #: 11016342
Client: G T Michelli
Address: 130 Brookhollow Esplanade

City & State: Harahan, LA 70123 5102
Date Received: 10 SEP 2008
Date Calibrated: 11 SEP 2008
Temperature Range: 21.49 to 22.25 °C
Pressure Range: 729.1 to 729.8 mmHg
Relative Humidity Range: 49 %
Air Density: 1.1405 to 1.1442 mg/cm³
Traceable Report #: 1451423
NIST Certificate #: 822/272801-06 822/274081-06
Tested By: 12
Procedure: Modified Substitution (W05-0023)
Contractor Req Recall Date: 2 Year
Primary Standard Calibration Date: 11/03/06 **Due:** 11/03/10
Description of Weights: 1mg-100g Polished Kit, Class "S", S/N 0113891
 Although there are two NIST numbers, one or both may apply.

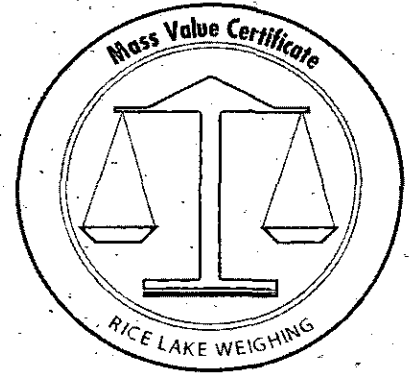

Nominal Value	Id.	Conventional Mass Corr.		Unc. K=2 (mg)	Tol. (mg)	Balance Used	Standard Set Used Calibrated/due MM-DD-YY/MM-DD-YY	Assumed Density (g/cm³)
		As Found (mg)	As Left (mg)					
1 mg		0.00244	0.00244	0.00072	0.014	501Q	K594Q 09-05-08/12-05-08	7.95
2 mg		0.00507	0.00507	0.00062	0.014	501Q	K594Q 09-05-08/12-05-08	7.95
3 mg		0.00174	0.00174	0.00061	0.014	501Q	K594Q 09-05-08/12-05-08	7.95
5 mg		0.00097	0.00097	0.00069	0.014	501Q	K594Q 09-05-08/12-05-08	7.95
10 mg		0.00917	0.00917	0.00094	0.014	501Q	K594Q 09-05-08/12-05-08	7.95
20 mg		0.00318	0.00318	0.00087	0.014	501Q	K594Q 09-05-08/12-05-08	7.95
30 mg		0.00119	0.00119	0.00094	0.014	501Q	K594Q 09-05-08/12-05-08	7.95
50 mg		-0.00017	-0.00017	0.00097	0.014	501Q	K594Q 09-05-08/12-05-08	7.95
100 mg		-0.0020	-0.0020	0.0014	0.025	501Q	K594Q 09-05-08/12-05-08	7.95
200 mg		0.0119	0.0119	0.0014	0.025	501Q	K594Q 09-05-08/12-05-08	7.95
300 mg		-0.0057	-0.0057	0.0014	0.025	501Q	K594Q 09-05-08/12-05-08	7.95
500 mg		-0.0155	-0.0155	0.0017	0.025	501Q	K594Q 09-05-08/12-05-08	7.95
1 g		0.0080	0.0080	0.0023	0.054	501Q	K594Q 09-05-08/12-05-08	7.95
2 g		0.0074	0.0074	0.0026	0.054	501Q	K594Q 09-05-08/12-05-08	7.95
3 g		0.0183	0.0183	0.0037	0.054	501Q	K594Q 09-05-08/12-05-08	7.95
5 g		0.0090	0.0090	0.0056	0.054	501Q	K594Q 09-05-08/12-05-08	7.95
10 g		-0.018	-0.018	0.013	0.074	676Q	K594Q 09-05-08/12-05-08	7.95
20 g		-0.003	-0.003	0.012	0.074	676Q	K594Q 09-05-08/12-05-08	7.95
30 g		0.044	0.044	0.020	0.074	1183Q	K594Q 09-05-08/12-05-08	7.95
50 g		0.053	0.053	0.021	0.12	1183Q	K594Q 09-05-08/12-05-08	7.95
100 g		-0.196	0.150	0.042	0.25	1183Q	K594Q 09-05-08/12-05-08	7.95

Check with your local state agency for certification of compliance on legal-for-trade items.

Prepared By:



230 West Coleman Street • Rice Lake, WI 54868 • USA
 TEL: 715-234-9171 • FAX: 715-234-6967

Dated 11 SEP 2008

Debbie Schieffer
 Debbie Schieffer Lab Supervisor

This report is not to be used to claim product endorsement by Rice Lake Weighing Systems or any agency of the U.S. Government. This document shall not be reproduced, except in full, without the written approval of Rice Lake Weighing Systems' Metrology Laboratory. The above uncertainty does not include a component for magnetic property or handling and use.