

RLWS *Mass Value* CERTIFICATE

Contractor:

G T Michelli
130 Brookhollow Esplanade
Harahan, LA 70123 5102

Purchase Order #:

11016340

Client:

G T Michelli

Address:

130 Brookhollow Esplanade

City & State:

Harahan, LA 70123 5102

Date Received:

10 SEP 2008

Date Calibrated:

11 SEP 2008

Temperature Range:

21.93 to 22.08 °C

Pressure Range:

729.8 to 730.9 mmHg

Relative Humidity Range:

49 %

Air Density:

1.1430 to 1.1442 mg/cm³

Traceable Report #:

1451425

NIST Certificate #:

822/272801-06 822/274081-06

Tested By:

12

Procedure:

Modified Substitution (WI05-0023)

Contractor Req Recall Date:

2 Year

Primary Standard Calibration Date:


11/03/06

Due: 11/03/10

Description of Weights:

100g-1kg Satin Finish Kit, Class "2", S/N S473

Although there are two NIST numbers, one or both may apply.

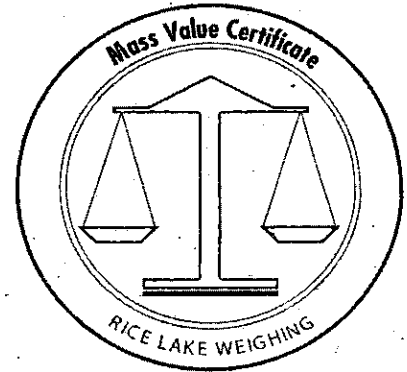

Nominal Value	Id.	Conventional Mass Corr.		Unc. K=2 (mg)	Tol. (mg)	Balance Used	Standard Set Used	Calibrated/due MM-DD-YY/MM-DD-YY	Assumed Density (g/cm ³)
		As Found (mg)	As Left (mg)						
100 g	J879	-0.114	-0.114	0.042	0.50	1183Q	K594Q	09-05-08/12-05-08	7.84
200 g	J878	0.159	0.159	0.053	1.0	619Q	K594Q	09-05-08/12-05-08	7.84
200 g	J877	0.189	0.189	0.053	1.0	619Q	K594Q	09-05-08/12-05-08	7.84
500 g	J876	0.239	0.239	0.086	2.5	619Q	K594Q	09-05-08/12-05-08	7.84
500 g	J875	0.046	0.046	0.086	2.5	619Q	K594Q	09-05-08/12-05-08	7.84
1 kg	J865	-1.29	-1.29	0.15	5.0	619Q	K594Q	09-05-08/12-05-08	7.84
1 kg	J866	-0.86	-0.86	0.15	5.0	619Q	K594Q	09-05-08/12-05-08	7.84
1 kg	J867	-1.10	-1.10	0.15	5.0	619Q	K594Q	09-05-08/12-05-08	7.84
1 kg	J868	-1.37	-1.37	0.15	5.0	619Q	K594Q	09-05-08/12-05-08	7.84

Check with your local state agency for certification of compliance on legal-for-trade items.

Prepared By:

RICE LAKE
WEIGHING SYSTEMS



Page 1 of 1 Page

Dated 11 SEP 2008
Debbie Schieffer
Debbie Schieffer Lab Supervisor

Commitment Beyond Measurement®
230 West Coleman Street • Rice Lake, WI 54868 • USA
TEL: 715-234-9171 • FAX: 715-234-6967

This report is not to be used to claim product endorsement by Rice Lake Weighing Systems or any agency of the U.S. Government.
This document shall not be reproduced, except in full, without the written approval of Rice Lake Weighing Systems' Metrology Laboratory.
The above uncertainty does not include a component for magnetic property or handling and use.

PN 38914 8/08