

Contractor:

G T Michelli Co Inc
130 Brookhollow Esplanade
Harahan, LA 70123-5102

Purchase Order #:

11016663

Client:

G T Michelli Co Inc

Address:

130 Brookhollow Esplanade

City & State:

Harahan, LA 70123 5102

Date Received:

08 JAN 2009

Date Calibrated:

09 JAN 2009

Temperature Range:

20.71 to 22.09 °C

Pressure Range:

732.7 to 732.9 mmHg

Relative Humidity Range:

49 %

Air Density:

1.1470 to 1.1531 mg/cm³

Traceable Report #:

1483394

NIST Certificate #:

822/272801-06 822/274081-06

Tested By:

12

Procedure:

Modified Substitution (WI05-0023)

Contractor Req Recall Date:

2 Year

Primary Standard Calibration Date:


11/03/06

Due: 11/03/10

Description of Weights:

1kg, 2-2kg, 5kg Polished Kit, Class "2", S/N T573

Although there are two NIST numbers, one or both may apply.

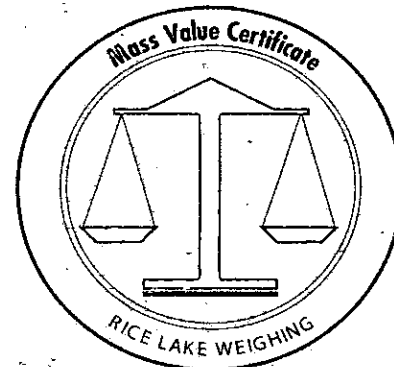

Nominal Value	Id.	Conventional Mass Corr.		Unc. K=2 (mg)	Tol. (mg)	Balance Used	Standard Set Used	Calibrated/due MM-DD-YY/MM-DD-YY	Assumed Density (g/cm ³)
		As Found (mg)	As Left (mg)						
1 kg		1.46	1.46	0.15	5.0	619Q	K594Q	12-02-08/03-02-09	7.84
2 kg		4.92	4.92	0.66	10	975Q	K594Q	12-02-08/03-02-09	7.84
2 kg	2	1.90	1.90	0.66	10	975Q	K594Q	12-02-08/03-02-09	7.84
5 kg		-5.33	-5.33	0.97	25	975Q	K594Q	12-02-08/03-02-09	7.84

Check with your local state agency for certification of compliance on legal-for-trade items.

Prepared By:



230 West Coleman Street • Rice Lake, WI 54868 • USA
TEL: 715-234-9171 • FAX: 715-234-6967

Dated 09 JAN 2009

Dan Demers
Dan Demers Metrologist