

130 Brookhollow
 Harahan, Louisiana, 70123
 Phone: 504-733-9822
 Fax: 504-734-0602
 www.michelli.com

Scales

Since 1947

Certificate of Calibration

Customer: G.T. Michelli Co., Inc. (Harahan)
Address: 130 Brookhollow Esplanade
City, State Zip: Harahan, LOUISIANA 70123


Certificate ID: 083150170091512
ISO Number: ISO9001:2000 cert#C2009-01862
Date: 12/15/2009

| | | | | |
|---------------------------------------|--------------------------------------|---------------------------------|-----------------------------------|-----------------------------------------------|
| Indicator Mfg. Weigh-Tronix | Base Mfg. Sensortronics | Cal Date 12/15/2009 | Scale ID 083150170 | Scale Location Mobile Lab - WCT-30k |
| Indicator Model E1010 | Base Model 65088S50K-1000 | Due Date 12/31/2010 | Scale Class III | Scale Range 0 - 30000 lb x 10 lb |
| Indicator Serial 083150170 | Base Serial 1528477 | Procedure Handbook 44 | Scale Status In Service | |
| Test Interval 12 Months | Customer Scale ID EQ# 1008 | | | |

EQUIPMENT CONDITIONS

[Working] Non-Working [Clean] Dirty Out of Level Out of Service In Storage

SHIFT TEST Shift Test Result: Pass Fail Adjust [Not Applicable]

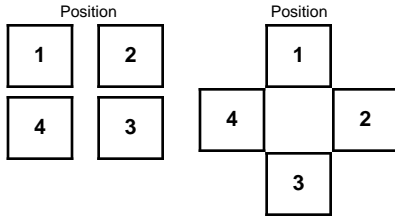

All tolerances calculated in conformance with Handbook 44 Table 6.

LOAD TEST

| Preliminary Load Test | | | |
|-----------------------|------------------|----------|-------|
| Test Wt. | Tolerance | Reading | Error |
| 10000 lb | 9980 - 10020 lb | 10000 lb | 0 lb |
| 20000 lb | 19980 - 20020 lb | 20020 lb | 20 lb |
| 30000 lb | 29970 - 30030 lb | 30030 lb | 30 lb |

In maintenance tolerance? [Yes] No

| Final Load Test | | | |
|-----------------|------------------|----------|-------|
| Test Wt. | Tolerance | Reading | Error |
| 10000 lb | 9980 - 10020 lb | 10000 lb | 0 lb |
| 20000 lb | 19980 - 20020 lb | 20000 lb | 0 lb |
| 30000 lb | 29970 - 30030 lb | 30000 lb | 0 lb |

In maintenance tolerance? [Yes] No

TEST INFORMATION

Test Weight Classification: Universal Test Stand
NIST Traceability Certificate Number: 31163L1008(COMP) Cal Date: 12/10/2008 Recal Date: 12/30/2010
Standards Used: Riehle UTM FS160 Compress (S# 042740254/R-46695-2)
Test Location: [Onsite] Offsite
Overall Result: Pass Fail [Adjust] No Test Performed No adjustment
Was the scale within customers required accuracy? [Y] N
Environmental Conditions: [Acceptable] Unacceptable
Comments / Notes: N/A
Technician: Lonnie Escude - License# LA-084 / MS-102

Equipment was calibrated with certified test weights or certified standards. Adjustments made to restore and/or maintain the accuracy of the equipment conform to the tolerances established by the National Institute of Standards and Technology as specified in Handbook 44, Section 2.20, or Manufacturer's Specifications. Best measurement of uncertainty calculated using a coverage factor of K=2. This provides confidence level of 95%. Reference GTM/TBL-IMS-782A. This certificate shall not be reproduced, except in full, without the written approval of the laboratory.